


# Certificate of Analysis

**Product** Exigo System Cleaner, RFID (1.9 L)  
**Product No** 1504503  
**Lot No** 2304-896  
**Manufacturing Date** 2023-04-11  
**Expiration Date** 2026-04-10

Test	Specification
pH	7,00 – 8,00
Conductivity (mS/cm)	15,25 – 17,00
Particles (PLT/RBC channel)	≤ 30

Actual values meet specifications.

Date: 2023-04-14

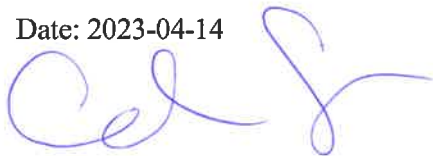

*Caroline Sparf*  
Quality Assurance

This product is intended for Laboratory use only unless otherwise specifically stated.  
All information in this document is property of Boule Medical AB.

