


Certificate of Analysis

Product Exigo System Cleaner, RFID (1.9 L)
Product No 1504503
Lot No 2505-322
Manufacturing Date 2025-05-22
Expiration Date 2028-05-21

Test	Specification
pH	7,00 – 8,00
Conductivity (mS/cm)	15,25 – 17,00
Particles (PLT/RBC channel)	≤ 30

Actual values meet specifications.

Date: 2025-05-27

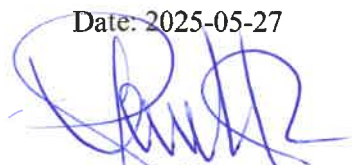

Pernilla Hammarstedt Rydberg
Quality Assurance

This product is intended for Laboratory use only unless otherwise specifically stated.
All information in this document is property of Boule Medical AB.

